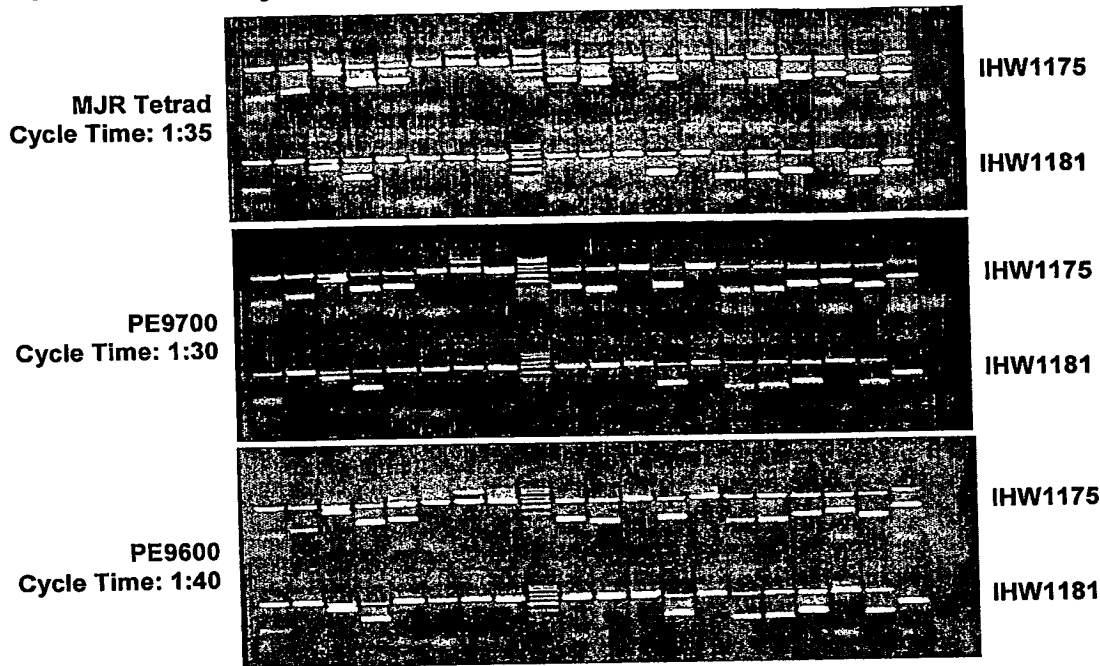


FIGURE 1

NK Panel Family 1416 Samples Amplified on Different Thermal Cyclers



1 x 95°C 2min, 30 x 94°C 20s, 63°C 20s, 72°C 1m30s

FIGURE 2

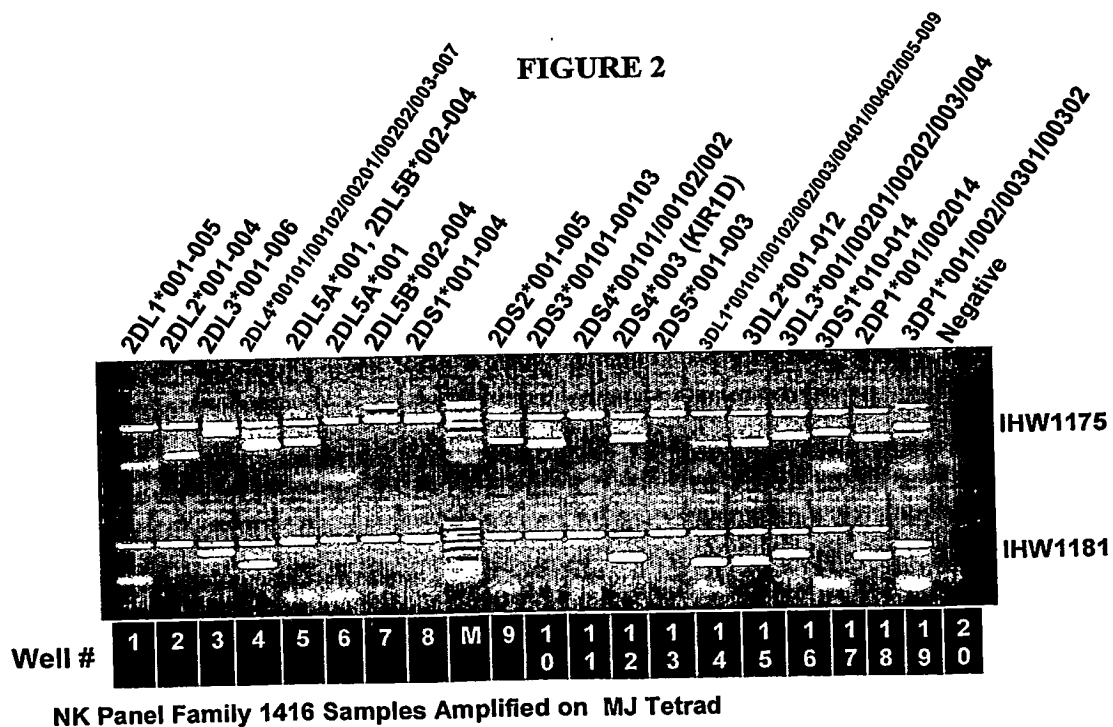
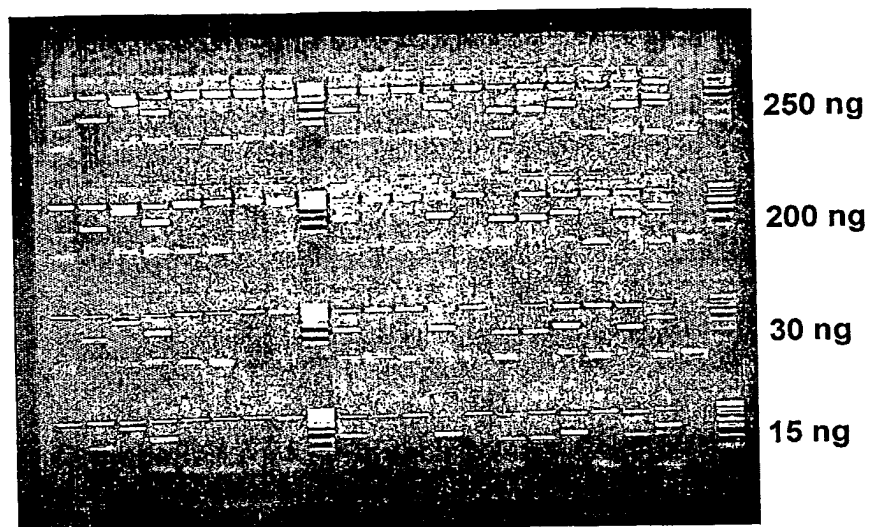
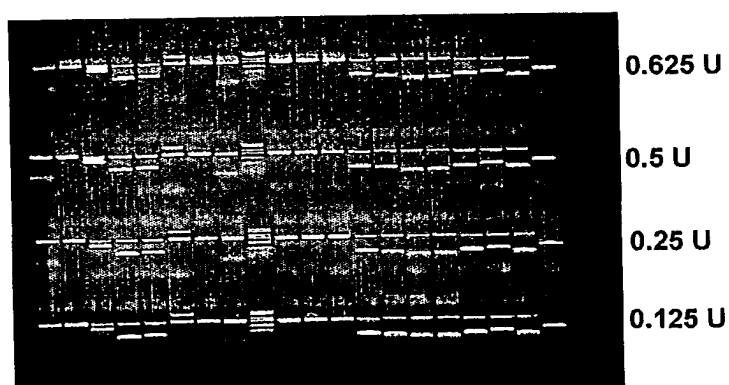


FIGURE 3**Different DNA Template Quantity**

1 x 95°C 2min, 30 x 94°C 20s, 63°C 20s, 72°C 1m30s

FIGURE 4**Different Taq Amount**

BEST AVAILABLE COPY

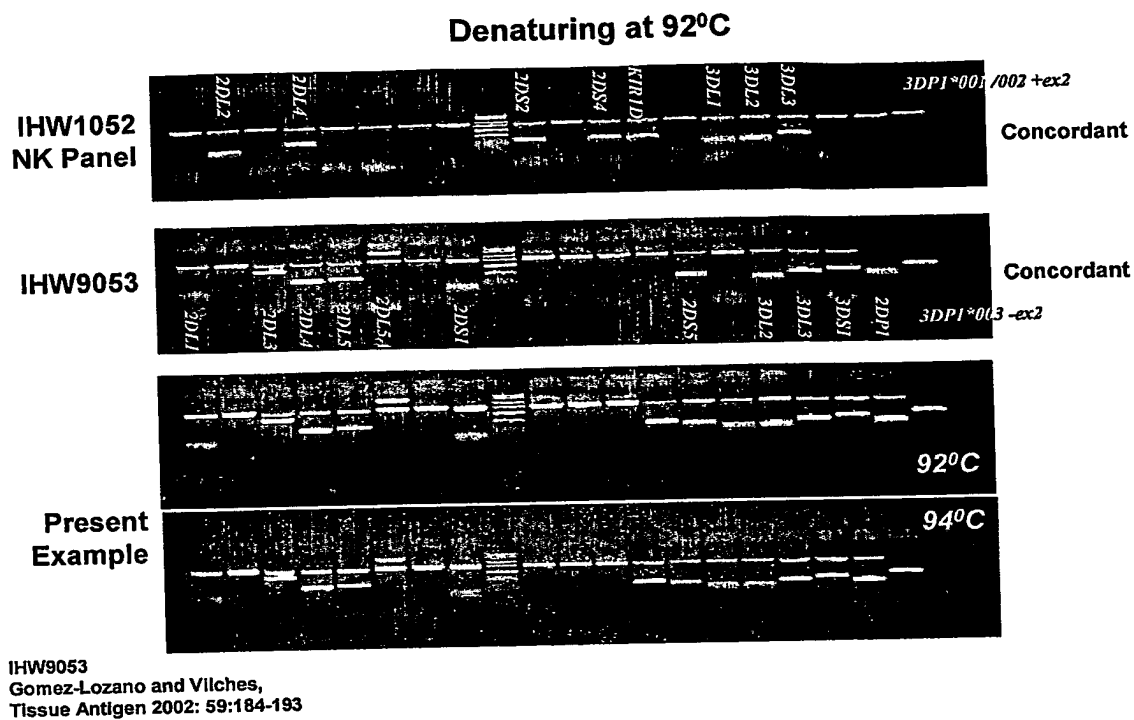
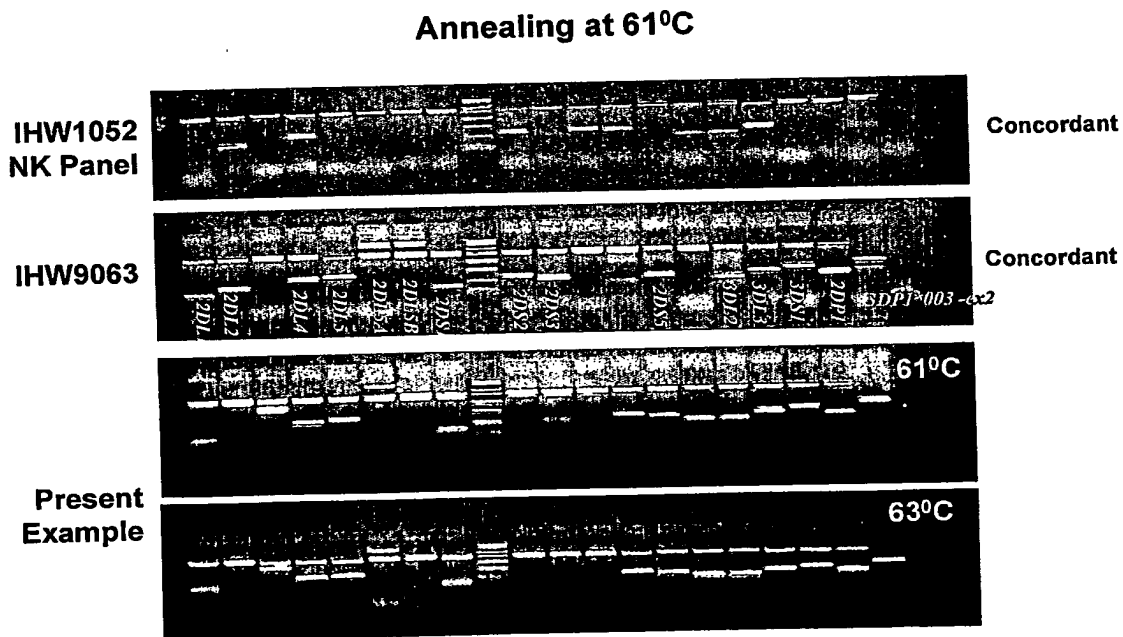
FIGURE 5**FIGURE 6****BEST AVAILABLE COPY**

FIGURE 7

Annealing at 65°C

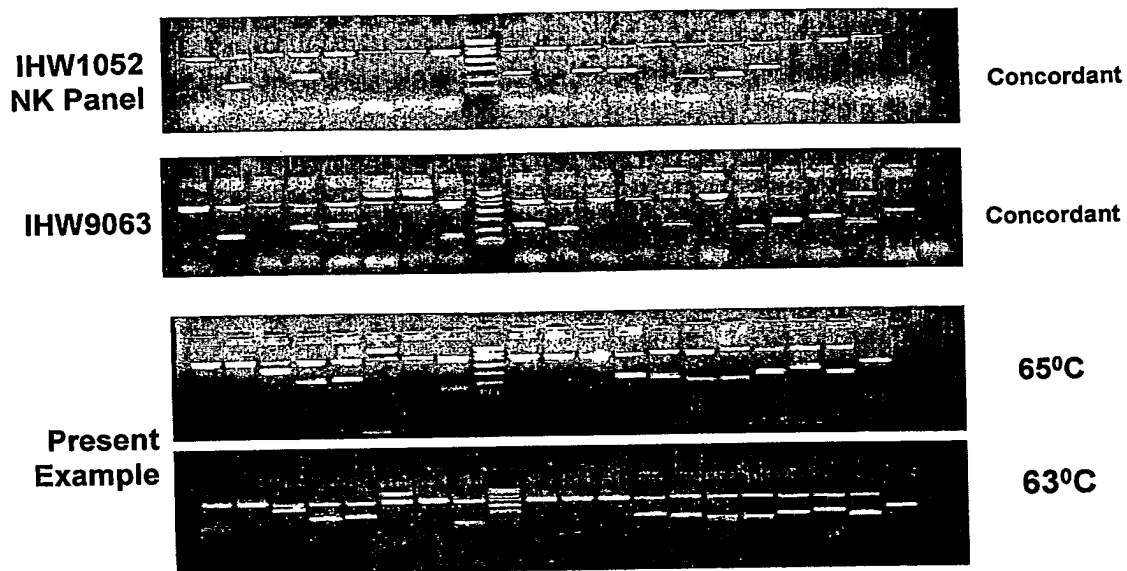
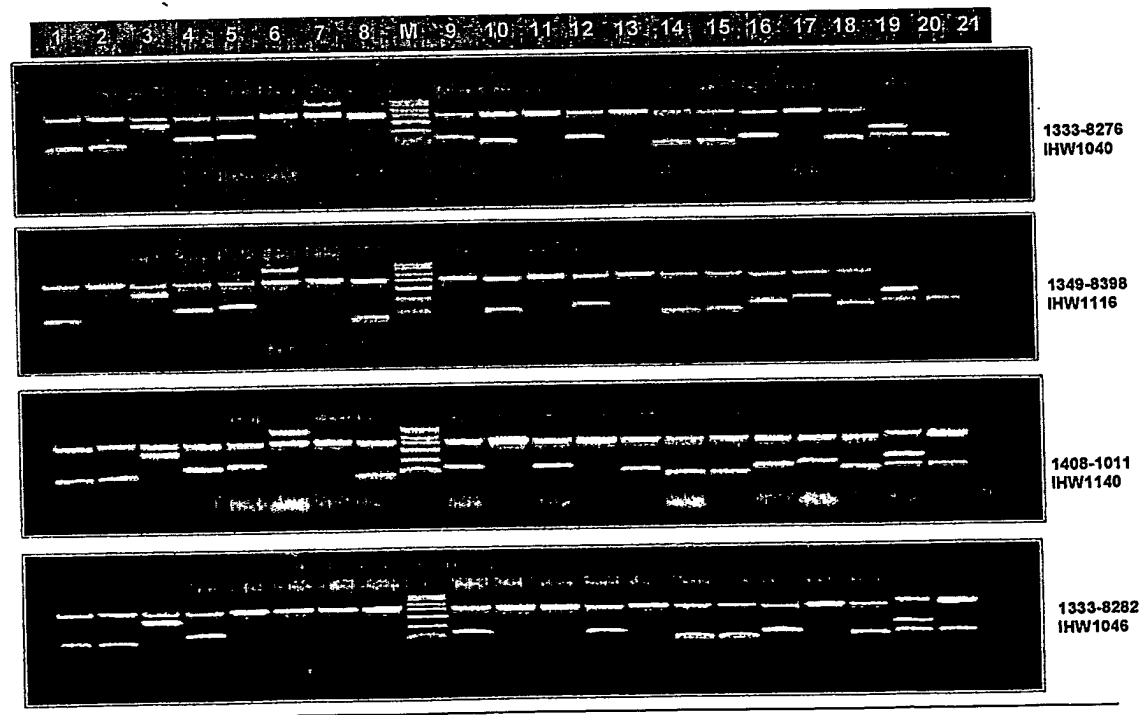


FIGURE 8



BEST AVAILABLE COPY